

Available online at [www.sciencedirect.com](http://www.sciencedirect.com)

# Resuscitation Plus

journal homepage: [www.elsevier.com/locate/resuscitation-plus](http://www.elsevier.com/locate/resuscitation-plus)

## Review

# Use of CPR feedback devices in resuscitation training: A systematic review and meta-analysis of randomized controlled trials



Yiqun Lin<sup>a,\*</sup>, Andrew Lockey<sup>b,c</sup>, Aaron Donoghue<sup>d</sup>, Robert Greif<sup>e,f</sup>,  
 Andrea Cortegiani<sup>g,h</sup>, Barbara Farquharson<sup>i</sup>, Fahad Javaid Siddiqui<sup>j</sup>, Arna Banerjee<sup>k</sup>,  
 Tasuku Matsuyama<sup>l</sup>, Adam Cheng<sup>m,n</sup>,  
 on behalf of the Education Implementation Team Task Force of the International Liaison  
 Committee on Resuscitation ILCOR<sup>1</sup>

## Abstract

**Objectives:** The use of cardiopulmonary resuscitation (CPR) feedback devices during training is increasing. This review evaluates whether incorporating CPR feedback devices in training improves patient survival, CPR quality in actual resuscitation, skill acquisition and retention after training.

**Methods:** This systematic review was part of the continuous evidence evaluation process of the International Liaison Committee on Resuscitation (ILCOR). We searched MEDLINE, EMBASE, and SCOPUS databases from inception to September 30, 2024, including randomized controlled trials (RCTs) in all languages (with an English abstract) comparing CPR training with and without feedback devices. Outcome included patient survival, quality of clinical performance in resuscitation, and CPR skill acquisition and retention. Non-RCT studies, unpublished work without peer review or animal studies were excluded. Risk of bias was assessed using Cochrane tools, and certainty of evidence was graded using the Grading of Recommendations Assessment, development and Evaluation (GRADE) approach. Standardized mean difference (SMD) were calculated and pooled effects were analyzed using random-effects models. PROSPERO CRD42023488130.

**Results:** We identified 20 RCTs with 4579 participants. Risks of bias ranged from low to critical (low: 8, moderate: 9, and critical: 3). No studies evaluated the patient survival, clinical performance in resuscitation or cost-effectiveness. Compared to no feedback, using CPR feedback devices during training significantly improved key quality metrics. Pooled effect sizes were 0.76 (95%CI 0.02 – 1.50) for mean compression depth (15 studies), 0.98 (95%CI: 0.10 – 1.87) for depth compliance (16 studies), 0.29 (95%CI: 0.10 – 0.48) for mean rate (17 studies), 0.44 (95%CI: 0.23 – 0.66) for rate compliance (9 studies), and 0.53 (95%CI: 0.31 – 0.75) for recoil compliance (10 studies) in favour of using feedback devices during training. Heterogeneity was large ( $I^2 > 50\%$ ) in all analyses. Planned subgroup analyses revealed no statistically significant interaction between healthcare professionals and laypersons. Using the GRADE approach, the certainty of evidence was downgraded for certain outcomes due to critical risk of bias for 3 studies and inconsistency but upgraded for strong association.

**Abbreviations:** BLS, basic life support, CPR, cardiopulmonary resuscitation, EIT, Education, Implementation and Teams, GRADE, Grading of Recommendations Assessment, Development and Evaluation, HCP, healthcare professional, ILCOR, International Liaison Committee on Resuscitation, PRISMA, Preferred Reporting Items for Systematic Review and Meta-Analysis, RCT, randomized controlled trial, ROB 2, Risk of Bias 2

\* Corresponding author at: KidSIM-ASPIRE Simulation Research Program, Alberta Children's Hospital, 28 Oki Dr NW, Calgary, Alberta, Canada T3B 6A8.

E-mail address: [jeffylin@hotmail.com](mailto:jeffylin@hotmail.com) (Y. Lin).

<sup>1</sup> The members of the Education Implementation Team Task Force of the International Liaison Committee on Resuscitation ILCOR are listed in Appendix 1 at the end of the article.

<https://doi.org/10.1016/j.resplu.2025.100939>

Received 29 January 2025; Received in revised form 7 March 2025; Accepted 10 March 2025

**Conclusion:** The use of CPR feedback devices during resuscitation training improves key quality metrics of CPR performance, with moderate to high certainty of evidence. However, further studies are needed to evaluate the impact on cost-effectiveness, clinical performance and patient outcomes.

**Keywords:** Resuscitation, CPR Feedback, Training, Basic Life Support, Medical Education

## Introduction

Cardiac arrest remains a major public health problem; with the incidence of out-of-hospital cardiac arrest varying from 30.0 to 97.1 cases per 100,000 population across the world.<sup>1–4</sup> The Utstein Formula for Survival emphasizes the critical role of effective resuscitation education in improving survival rates for cardiac arrest victims.<sup>5</sup> However, the deterioration of CPR skills following resuscitation training remains a persistent issue.<sup>6</sup> Developing strategies to enhance the acquisition and retention of CPR skills could significantly improve the quality of resuscitation efforts during cardiac arrest, ultimately leading to better patient outcomes.

Recent scientific statements highlight a growing trend in the use of CPR feedback devices during resuscitation training courses.<sup>7</sup> The use of CPR feedback devices addresses the issue of poor visual assessment skills amongst healthcare providers and CPR instructors. Earlier reviews suggested that CPR feedback devices may improve short-term educational outcomes.<sup>8</sup> Since then, new international resuscitation guidelines have been published, introducing optimal targets for compression depth and rate to enhance resuscitation outcomes.<sup>9,10</sup> Technological advancements now enable the objective measurement of CPR quality, providing precise, quantifiable data that can be synthesized to draw stronger, evidence-based conclusions.

Furthermore, a substantial number of new studies, including randomized controlled trials, have been published on this topic in recent years. These studies offer high-quality evidence, highlighting the need for an updated and comprehensive analysis to inform current practice and training standards. In this systematic review, we aim to determine whether the use of CPR feedback devices during resuscitation training, compared to training without such devices, improves CPR skill acquisition, skill retention, clinical performance quality during actual resuscitations, and patient survival.

## Methods

### Eligibility criteria

Members of the Education, Implementation and Teams (EIT) Task Force of the International Liaison Committee on Resuscitation (ILCOR) conducted this systematic review as part of the continuous evidence evaluation process of resuscitation literature informing international consensus treatment recommendations.<sup>11,12</sup> The review is reported in compliance with the Preferred Reporting Items for Systematic Review and Meta-Analysis (PRISMA) guidelines (Supplementary I),<sup>13</sup> and was registered with the Prospective Registry for Systematic Reviews (PROSPERO CRD42023488130). The research question was structured using the 'PICOST' (Population, Intervention, Comparison, Outcome, Study Design, Timeframe) format as per ILCOR evidence reviews:

**Population:** All laypersons and healthcare professionals receiving resuscitation training.

**Intervention:** Use of CPR feedback/guidance device during resuscitation training.

**Comparison:** No use of CPR feedback / guidance device during resuscitation training.

**Outcomes:** Patient Survival [Critical], skill performance in real resuscitation [Critical], cost-effectiveness [Important], skills acquisition [Important] and retention [Important] (i.e. CPR quality, chest compression depth, rate and recoil).

**Study Design:** Randomized controlled trials (RCTs) were eligible for inclusion. All relevant publications in any language were included as long as an English abstract was available.

**Timeframe:** Inception to September 30, 2024.

All included studies should use feedback devices in a resuscitation training course or simulated resuscitation event for the purpose of training and education only. Non-randomized studies, unpublished studies (without peer review) and animal studies were excluded in this review.

### Definitions

For this systematic review, we defined CPR feedback devices as any tool that evaluates performance and provides information (audio, visual or both) about the quality of chest compressions, or offer guidance (i.e. such as a metronome) to improve performance metrics such as compression depth, rate, and chest recoil.

### Information sources and search strategy

We utilized a search strategy developed in conjunction with an information specialist (CM) using (but not limited to) the following key terms: "cardiopulmonary resuscitation", "CPR", "basic life support", "advanced life support", "cardiac arrest", "chest compressions", "feedback device", "training" and searched Medline, Embase, and Scopus databases from inception until September 30, 2024. The detailed search strategy is shown in Supplementary II. Grey literature was not searched. Reference lists of identified studies and review articles were scanned to identify additional relevant publications.

### Study selection

Rayyan software (a web-based software for systematic reviews) was used to detect duplicates, with one reviewer (YL) screening and removing all relevant duplicates. Five pairs of reviewers independently (AC, YL; RG, TM; AD, AB; AL, FS; AC, BF) screened titles and abstracts and excluded all papers not meeting eligibility criteria. Disagreements amongst reviewer pairs were resolved via discussion to reach a consensus. In the rare instance when a consensus was not reached, full text of the paper was obtained for review. The full texts of remaining papers were independently reviewed for eligibility by four pairs of reviewers (AC, AB; TM, AL; YL, FS; AD, AB). The remaining disagreements were discussed amongst reviewer pairs to reach consensus on the final group of articles.

### Data extraction

After identification of the final group of articles, four pairs of reviews (AC, AB; TM, AL; YL, FJS; AD, AB) independently extracted relevant data from all the relevant articles into an Excel spreadsheet. Extracted data was double checked, with discrepancies resolved through review and discussion. Data extracted included author, publication year, country, study design, population, sample size, intervention and comparison, outcome measures, and results.

### Risk of bias assessment

Four pairs of reviewers (AC, AB; TM, AL; YL, FS; AD, AB) independently assessed the included papers for risk of bias using the Risk of Bias 2 (RoB 2) tool for RCTs.<sup>14</sup> Disagreements between reviewers was resolved by discussion to reach consensus.

### Synthesis of results

The overall certainty of evidence was assessed using the Grading of Recommendations Assessment, Development and Evaluation (GRADE) methodology. EIT task force members discussed the extracted data and results tables on several virtual conference calls to craft treatment recommendations and identify key insights and future opportunities for research.<sup>15,16</sup>

Means and standard deviations or odds ratios/risk differences reported by the included studies were converted to standardized mean differences (SMD, Hedges' *g* effect size). For studies that reported medians and interquartile ranges, the effect size was estimated under the assumption of a normal data distribution. If insufficient information was available to calculate an effect size, the authors were contacted via email to request the missing data. The  $\chi^2$  test and  $I^2$  statistic were used to assess inconsistency (heterogeneity) across studies. Due to the high heterogeneity observed in most analyses, random-effects models were employed to pool the effect sizes. Planned subgroup analyses were performed based on the type of trainees (healthcare professionals

vs. lay persons), with statistical significance of interactions evaluated using the *z* test. Some planned subgroup analyses were not conducted due to insufficient data (e.g. corrective feedback vs guidance feedback, incorporating feedback with other instructional design, gender, age and race). Forest plots were used to visually display the results of individual studies and synthesis. All analyses were conducted using R software (version 4.3.0) and the "meta" package.<sup>17</sup> A two-sided alpha level of 0.05 was used to define statistical significance. Certainty of evidence was assessed using the Grading of Recommendations Assessment, development and Evaluation (GRADE) approach.

## Results

### Study characteristics

Our initial literature search yielded 9756 citations. After removing 3440 duplicates, 6316 articles underwent title and abstract screening. From these, 115 articles were identified for full-text review, resulting in the inclusion of 18 studies. An additional 2 studies were identified via search of references lists of relevant articles, bringing the total to 20 studies (4579 participants) included in the final analysis, with publication years ranging from 2007 to 2023. (Fig. 1).

None of the included studies evaluated the impact of CPR feedback devices during resuscitation training on patient survival outcomes, quality of performance in actual resuscitation or cost-effectiveness of training. All 20 studies examined the CPR skills at the conclusion of the courses<sup>18–37</sup>, and 8 of them also examined the CPR skill retention 3 months post-training<sup>18,22,25,28,29,33,34,37</sup>. Among the 20 studies, 17 were conducted in healthcare professionals<sup>18,20–25,27–29,31–37</sup>, while 3 focused on lay persons.<sup>19,26,30</sup> (Table 1). Regarding the risk of bias, 8 studies rated as having minor concerns<sup>19,22,23,26,27,29,30,36</sup>, 9 studies having some concerns<sup>18,21,24,25,28,32,34,35,37</sup>, and 3 studies as having serious

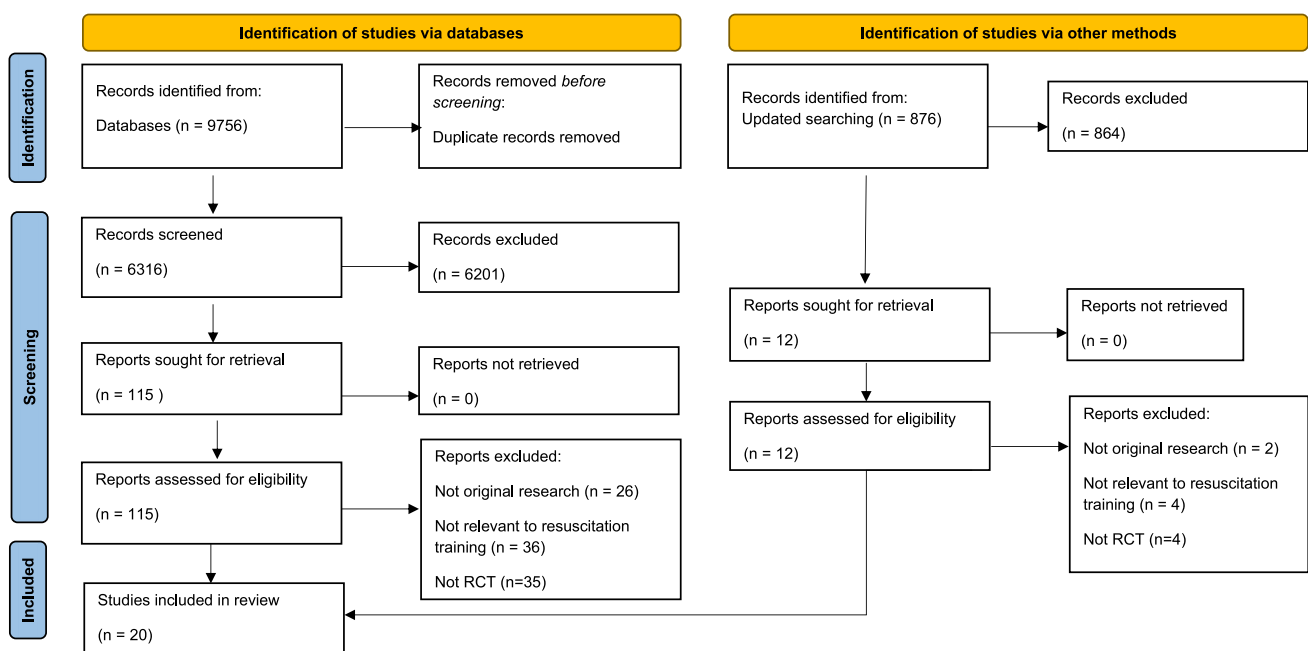


Fig. 1 – PRISMA flow diagram.

**Table 1 – Summary of included studies.**

| Study                 | Country      | Mean depth | Mean rate | Depth compliance | Rate compliance | Recoil compliance | Overall score * | Overall quality | Provider | Skill Acquisition | Skill Retention |
|-----------------------|--------------|------------|-----------|------------------|-----------------|-------------------|-----------------|-----------------|----------|-------------------|-----------------|
| Allan 2013            | Canada       | +          | +         | –                | –               | –                 | –               | –               | HCP      | +                 | +               |
| Cortegiani 2017       | Italy        | +          | +         | +                | +               | +                 | +               | –               | LP       | +                 | –               |
| Ghaderi 2023          | Iran         | –          | –         | +                | +               | +                 | –               | –               | HCP      | +                 | –               |
| Gonzalez-Santano 2020 | Spain        | +          | +         | +                | –               | +                 | +               | –               | HCP      | +                 | –               |
| Jang 2020             | Korea        | +          | +         | +                | –               | –                 | –               | –               | HCP      | +                 | +               |
| Jiang 2024            | China        | +          | +         | +                | +               | –                 | –               | –               | HCP      | +                 | –               |
| Kardong-Edgren 2010   | US           | +          | +         | +                | –               | –                 | –               | –               | HCP      | +                 | –               |
| Katipoglu 2021        | Poland       | +          | +         | +                | +               | +                 | +               | –               | HCP      | +                 | +               |
| Kong 2020             | Korea        | +          | +         | +                | –               | +                 | +               | –               | LP       | +                 | –               |
| Labuschagne 2022      | South Africa | –          | +         | +                | +               | –                 | +               | –               | HCP      | +                 | –               |
| Lee 2023              | Taiwan       | –          | –         | +                | +               | +                 | +               | –               | HCP      | +                 | +               |
| Lin 2018              | Canada       | –          | –         | +                | +               | +                 | –               | +               | HCP      | +                 | +               |
| Meng 2021             | China        | –          | +         | +                | –               | –                 | –               | –               | LP       | +                 | –               |
| Min 2016              | Korea        | +          | +         | +                | –               | –                 | –               | –               | HCP      | +                 | –               |
| Pavo 2016             | Switzerland  | +          | +         | +                | –               | –                 | +               | –               | HCP      | +                 | –               |
| Spooner 2007          | UK           | +          | +         | –                | –               | –                 | –               | –               | HCP      | +                 | +               |
| Suet 2020             | France       | +          | +         | –                | –               | +                 | +               | –               | HCP      | +                 | +               |
| Sutton 2011           | US           | +          | +         | –                | –               | –                 | –               | +               | HCP      | +                 | –               |
| Wagner 2019           | Canada       | +          | +         | +                | +               | +                 | –               | –               | HCP      | +                 | –               |
| Zhou 2020             | China        | +          | +         | +                | +               | +                 | –               | –               | HCP      | +                 | +               |

\* Overall chest compression quality measured by software with limited validity evidence.

\*\* Overall chest compression quality measured dichotomously (Overall quality considered good if depth, rate and recoil all meeting guidelines)HCP: healthcare professionals; LP: Lay persons.

| Study                 | Randomization | Deviations from intended intervention | Outcome data missing | Measurement of outcome | Selection of reported results | Overall |
|-----------------------|---------------|---------------------------------------|----------------------|------------------------|-------------------------------|---------|
| Allan 2013            | Unclear       | Low                                   | Low                  | Low                    | Low                           | Some    |
| Cortegiani 2017       | Low           | Low                                   | Low                  | Low                    | Low                           | Minor   |
| Ghaderi 2023          | High          | Low                                   | Low                  | Low                    | Low                           | Serious |
| Gonzalez-Santano 2020 | Unclear       | Low                                   | Low                  | Low                    | Low                           | Some    |
| Jang 2020             | Low           | Low                                   | Low                  | Low                    | Low                           | Minor   |
| Jiang 2024            | Low           | Low                                   | Low                  | Low                    | Low                           | Minor   |
| Kardong-Edgren 2010   | Unclear       | Low                                   | Low                  | Low                    | Low                           | Some    |
| Katipoglu 2021        | Unclear       | Unclear                               | Low                  | Low                    | Low                           | Some    |
| Kong 2020             | Low           | Low                                   | Low                  | Low                    | Low                           | Minor   |
| Labuschagne 2022      | Low           | Low                                   | Low                  | Low                    | Low                           | Minor   |
| Lee 2023              | Low           | Low                                   | Unclear              | Low                    | Low                           | Some    |
| Lin 2018              | Low           | Low                                   | Low                  | Low                    | Low                           | Minor   |
| Meng 2021             | Low           | Low                                   | Low                  | Low                    | Low                           | Minor   |
| Min 2016              | High          | Low                                   | Low                  | Low                    | Low                           | Serious |
| Pavo 2016             | Low           | Low                                   | Low                  | Low                    | Unclear                       | Some    |
| Spooner 2007          | Unclear       | Low                                   | Unclear              | Low                    | Unclear                       | Serious |
| Suet 2020             | Unclear       | Low                                   | Low                  | Low                    | Low                           | Some    |
| Sutton 2011           | Unclear       | Low                                   | Low                  | Low                    | Low                           | Some    |
| Wagner 2019           | Low           | Low                                   | Low                  | Low                    | Low                           | Minor   |
| Zhou 2020             | Unclear       | Low                                   | Low                  | Low                    | Low                           | Some    |

**Fig. 2 – Risk of bias assessment.**

concerns.<sup>20,31,33</sup> (Fig. 2). Using the GRADE approach, the certainty of evidence was downgraded for certain outcomes due to critical risk of bias for 3 studies and inconsistency but upgraded for strong asso-

ciation. The overall certainty of evidence was moderate to high. A detailed description of certainty of evidence is presented in Supplementary III.

### Chest compression depth


Fifteen RCTs involving 4185 participants evaluated the effect of CPR feedback devices on objectively measured mean compression depth.<sup>18–19,21–26,31–37</sup> The results indicated that participants trained with feedback devices achieved significantly greater mean compression depth compared to those trained without them (SMD = 0.76, 95% CI: 0.02–1.50,  $p = 0.04$ ,  $I^2 = 94\%$ ) immediately after training. The difference in effect size between the healthcare professionals and lay persons were not statistically significant ( $p = 0.10$ ). (Fig. 3, Supplementary IV-Fig. 1). Five studies comprising 431 participants showed the effect of feedback devices on mean compression depth skill retention. The results indicated no significant difference in mean compression depth at 3 months post training. (SMD = 1.56, 95%CI: -0.32 – 3.43,  $p = 0.10$ ,  $I^2 = 97$ ). (Fig. 4, Supplementary IV-Fig. 2).

Sixteen RCTs involving 4304 participants examined the effect of CPR feedback devices during resuscitation training on compression depth compliance.<sup>36,37,19–32</sup> Compression depth compliance was


quantitatively measured as the percentage of compressions meeting the resuscitation guidelines during assessment. The use of CPR feedback devices during training had a large impact on depth compliance (SMD = 0.98, 95% CI: 0.10–1.87,  $p = 0.03$ ,  $I^2 = 94\%$ ). The difference in effect size between the healthcare professionals (SMD 1.14, 95%CI: 0.04–2.24) and the lay persons (SMD 0.17, 95%CI: 0.01 – 0.32) was not statistically significant ( $p = 0.09$ ). (Fig. 3, Supplementary IV-Fig. 3) Furthermore, five RCTs with 478 participants reported a large effect size of feedback devices on depth compliance three months after the training (SMD = 1.77, 95%CI: 0.25 – 3.30,  $p = 0.02$ ,  $I^2 = 97\%$ ). (Fig. 4, Supplementary IV-Fig. 4).

### Chest compression rate

Seventeen RCTs involving 4,327 participants assessed the effect of CPR feedback devices on objectively measured mean compression rate.<sup>18,19,21–27,30–37</sup> Participants trained with feedback devices had a significantly lower mean compression rate compared to those trained

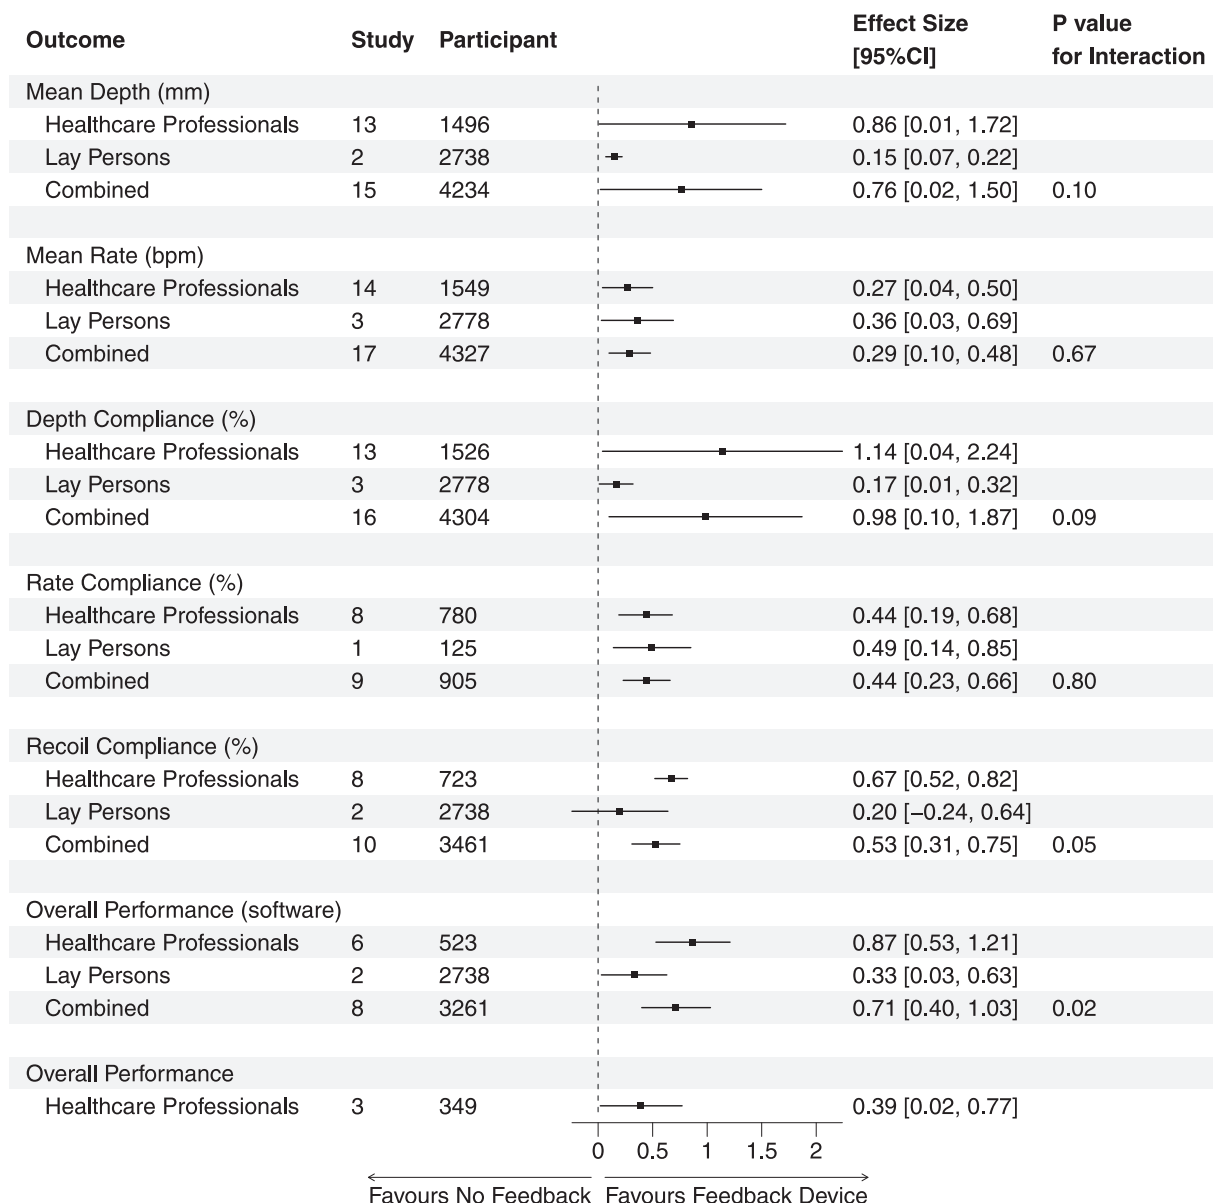

**Fig. 3 – Effect of feedback device use during training on CPR quality immediately post-training.**



**Fig. 4 – Effect of feedback device use during training on CPR quality 3 months post-training.**

without them, as participants in the non-feedback group tended to compress too quickly ( $>120$  bpm) (SMD =  $-0.29$ , 95% CI:  $-0.49$  to  $-0.10$ ,  $p < 0.01$ ,  $I^2 = 73\%$ ). Subgroup analysis showed the effect of the feedback device on mean compression rate was not statistically significant between healthcare professionals and lay persons ( $p = 0.67$ ). (Fig. 3' Supplementary IV–Fig. 5). Five RCTs involving 431 participants reported a non-significant difference on mean compression rate at 3 months post-training (SMD =  $-0.67$ , 95%CI:  $-1.45$  –  $0.11$ ,  $p = 0.09$ ,  $I^2 = 93\%$ ). (Fig. 4' Supplementary IV–Fig. 6).

Additionally, nine RCTs involving 905 participants examined the effect of CPR feedback devices during resuscitation training on compression rate compliance.<sup>19,20,23,25,36,37,27–29</sup> Compression rate compliance was quantitatively measured as the percentage of compressions within the guideline-recommended rate of 100–120 bpm. CPR feedback devices had a substantial impact on rate compliance (SMD =  $0.45$ , 95% CI:  $0.23$ – $0.66$ ,  $p < 0.01$ ,  $I^2 = 61\%$ ) immediately after the training. Subgroup analysis showed the effect of the feedback device on rate compliance was not statistically significant between healthcare professionals and lay persons ( $p = 0.80$ ) (Fig. 3' Supplementary IV–Fig. 7). Four RCTs with 383 participants indicated a large effect on rate compliance at 3 months post-training (SMD  $0.95$ , 95%CI:  $0.25$  –  $1.66$ ,  $p < 0.01$ ,  $I^2 = 90\%$ ) (Fig. 4' Supplementary IV–Fig. 8).

### Chest recoil

Ten RCTs with 3,496 participants assessed the effect of CPR feedback devices during training on chest recoil.<sup>25–26,28–29,34,36–37,19–21</sup> Chest recoil was quantitatively measured as the percentage of compressions with complete chest recoil. CPR feedback had a significant effect on recoil compliance (SMD =  $0.53$ , 95% CI:  $0.31$ – $0.75$ ,  $p < 0.01$ ,  $I^2 = 87\%$ ) immediately after the training. Subgroup analysis showed that the effect of the feedback device on recoil compliance was significantly higher in healthcare professionals than in the lay persons. ( $p = 0.05$ ). (Fig. 3' Supplementary IV–Fig. 9). Five RCTs involving 424 participants showed the effect of feedback device on recoil compliance remained significant 3 months post-training (SMD  $0.57$ , 95%CI:  $0.38$  –  $0.77$ ,  $p < 0.01$ ,  $I^2 = 0\%$ ). (Fig. 4' Supplementary IV–Fig. 10).

### Overall quality of CPR

Eight RCTs involving 3261 participants evaluated the effect of CPR feedback devices on overall CPR quality during resuscitation training.<sup>19,21,34,36,25–28</sup> Overall quality of CPR was assessed by computer

software integrating all three metrics of chest compression (depth, rate and recoil) with limited validity evidence. The results showed that the use of feedback devices significantly improved the overall quality of CPR, with a pooled effect size of  $0.71$  (95% CI:  $0.40$ – $1.05$ ,  $p < 0.01$ ,  $I^2 = 86\%$ ). Subgroup analysis showed that the effect of the feedback device on the overall CPR score was significantly higher in the healthcare professionals than in the lay persons ( $p = 0.02$ ). (Fig. 3' Supplementary IV–Fig. 11) In the 2 RCTs with 129 participants examining overall CPR skill retention, the effect of feedback device remained significant (SMD  $0.75$ , 95%CI:  $0.39$  –  $1.11$ ,  $p < 0.01$ ,  $I^2 = 0\%$ ). (Fig. 4' Supplementary IV–Fig. 12).

Three randomized controlled trials (RCTs) with 349 participants evaluated the effect of CPR feedback devices on overall CPR quality during resuscitation training.<sup>29,32,35</sup> CPR quality was assessed dichotomously, based on whether compression depth, rate, and recoil all met guideline standards. The use of feedback devices significantly improved the overall quality of CPR, with a pooled risk difference of  $0.19$  (95% CI:  $0.01$ – $0.38$ ,  $p = 0.04$ ,  $I^2 = 78\%$ ), which is equivalent to an effect size of  $0.39$  (95%CI:  $0.02$  –  $0.77$ ). (Supplementary IV–Fig. 13).

## Discussion

This systematic review on randomized controlled trials highlights the impact of using CPR feedback devices during resuscitation training on learning outcomes. By synthesizing the results of 20 randomized controlled trials, we demonstrated that incorporating feedback devices during resuscitation training significantly improves CPR skill acquisition and retention across all metrics of CPR quality for both healthcare professionals and lay persons.

Traditional Basic Life Support training that lacks CPR feedback devices fails in delivering objective feedback and in the accurate measurement of CPR quality. In these courses, CPR quality is typically assessed visually by an instructor, which has been proven inaccurate, even among experienced providers in acute care units.<sup>38</sup> This often leads to an overestimation of CPR quality, giving false reassurance to learners that are performing poorly.<sup>39</sup> In all forms of psychomotor skill learning, accurate feedback from an external source is crucial for correct skill development, as it provides learners with information beyond their inherent awareness.<sup>40</sup> A previous systematic review of 8 manikin studies investigating the impact of real-time feedback during resuscitation training reported mixed results.<sup>8</sup>



Despite the heterogeneity in outcome measures, most evidence supported use the feedback during CPR training to improve skill acquisition. However, few studies in that review have objectively measured CPR performance. Our review, in contrast addresses this gap by conducting *meta*-analyses on the CPR metrics objectively assessed at the conclusion of the course.

CPR feedback devices are both feasible and practical for use in training programs. While the mandatory use of feedback devices may potentially pose a financial barrier in some lower resource settings, the availability of low-cost options helps to mitigate this concern.<sup>41</sup> Feedback devices have been used in resuscitation training programs for years, and the growing body of literature across the world underscores their acceptability and practicality among key stakeholders<sup>42,43</sup>. Moreover, numerous studies and reviews demonstrate their effectiveness during real resuscitation events,<sup>43,44</sup> further validating their role in training. If feedback devices are valuable in improving outcomes during real resuscitation, integrating them into simulation training programs is both logical and essential.

We observed that the effect of CPR feedback during training appeared larger in healthcare professionals than on laypersons, though this difference was not statistically significant. This trend could partially be explained by adult learning theory and cognitive load theory<sup>45,46</sup>. Healthcare professionals, driven by intrinsic motivation and prior knowledge, engage deeply with feedback to refine their skills, as they see its relevance to their professional roles. Lay persons, often starting without prior CPR knowledge, focus on acquiring basic skills.<sup>45</sup> Based upon cognitive load theory,<sup>46</sup> interpreting CPR feedback on performance can increase extraneous load during training, which refers to cognitive effort unrelated to the primary learning task. For lay persons, processing real-time feedback from CPR devices requires mental resources to understand and act on the information, often competing with their focus on mastering basic skills like chest compressions. This additional demand can overwhelm their cognitive capacity, making it harder to concentrate on the essential aspects of CPR performance. These findings suggest the need to tailor training resources: feedback devices can help healthcare professionals maintain precision, while simpler tools and instructional design may better suit lay persons.

Our systematic review demonstrated that the use of CPR feedback devices during resuscitation training significantly improved CPR skill retention, which is a key determinant of real-world performance. Feedback devices provide immediately, objective guidance, reinforcing correct techniques and helping learners develop habits that persist beyond the training environment. While no direct evidence was identified linking the use of feedback devices during training to improved patient outcomes, there is a clear “chain of evidence”<sup>47</sup> logically connecting these elements. Feedback devices enhance CPR training by helping participants achieve guideline-compliant chest compressions, including proper depth, rate, and recoil. High-quality CPR, in turn, has been shown to significantly improve survival rates and neurological outcomes in cardiac arrest victims.<sup>48–50</sup> Therefore, improvements in training quality facilitated by feedback devices are likely to lead to better real-world CPR performance and, ultimately, better survival outcomes for cardiac arrest patients.

### **Limitations, knowledge gaps, and future research**

Our review has several limitations. First, we failed to identify any studies examining CPR quality in real clinical care or patient outcomes. Second, despite of inclusion of randomized trials only, the heterogeneity among the studies remains high in this review. Third,

we did not find evidence to address the cost-effectiveness of the feedback device used during resuscitation. Future research should also consider examining the relative and synergistic effect of CPR feedback device use when combined with other instructional design and educational strategies (e.g. spaced learning or deliberate practice). The return on investment associated with implementing CPR feedback device during resuscitation training needs further exploring. Further studies should explore transfer of CPR skills to the real clinical environment (e.g. CPR quality during real cardiac arrest event), which would further clarify the true effectiveness of the CPR feedback device use during resuscitation training.

## **Conclusion**

CPR feedback device used during resuscitation training significantly improve the CPR quality of the learners for both skill acquisition and retention. CPR feedback devices should be used during resuscitation training for both healthcare professionals and lay persons.

## **Other disclosures**

None.

## **Ethical approval**

Not applicable.

## **Disclaimers**

None.

## **CRedit authorship contribution statement**

**Yiqun Lin:** Writing – review & editing, Writing – original draft, Methodology, Investigation, Formal analysis, Data curation. **Andrew Lockey:** Writing – review & editing, Methodology, Investigation, Data curation, Conceptualization. **Aaron Donoghue:** Writing – review & editing, Methodology, Data curation, Conceptualization. **Robert Greif:** Writing – review & editing, Supervision, Methodology, Investigation, Data curation, Conceptualization. **Andrea Cortegiani:** Writing – review & editing, Methodology, Data curation, Conceptualization. **Barbara Farquharson:** Writing – review & editing, Methodology, Data curation, Conceptualization. **Fahad Javaid Siddiqui:** Writing – review & editing, Methodology, Data curation, Conceptualization. **Arna Banerjee:** Writing – review & editing, Methodology, Data curation, Conceptualization. **Tasuku Matsuyama:** Writing – review & editing, Methodology, Data curation, Conceptualization. **Adam Cheng:** Writing – review & editing, Writing – original draft, Supervision, Methodology, Data curation, Conceptualization.

## **Funding**

This work has been supported using public funds via the American Heart Association.

## Declaration of competing interest

The authors declare the following financial interests/personal relationships which may be considered as potential competing interests: YL, AL, AD, RG, AC (Andrea Cortegiani), BF, TM and AC (Adam Cheng) are members of the ILCOR EIT Task Force (RG is chair, AC is vice-chair). RG is the European Resuscitation Council Director of Guidelines and ILCOR, AL is Vice President of Resuscitation Council UK. AC, AL, and RG are Editorial Board members of Resuscitation Plus.

## Acknowledgements

The authors acknowledge the assistance provided by Caitlin McClurg the librarian at the University of Calgary for building up the searching strategy. The following ILCOR EIT Task Force members are acknowledged as collaborators in this systematic review: Cristian Abelairas-Gomez, Katherine Allan, Jan Breckwoldt, Kathryn Eastwood, Ming-Ju Hsieh, Tracy Kidd, Ying-Chih Ko, Kasper G Lauridsen, Sabine Nabecker, Kevin Nation, Alexander Olaussen, Sebastian Schnaubelt, Taylor Sawyer, Chih-Wei Yang, and Joyce Yeung. ChatGPT, a language model developed by OpenAI in San Francisco, CA, USA, was used for grammar and language editing in this manuscript. The authors reviewed and approved all suggestions to ensure accuracy and clarity.

## Data availability statement

The data collection forms, extracted data, and analytic codes are available from the corresponding author upon reasonable request.

## Appendix 1

\*Collaborators form the ILCOR Task Force the Education Implementation Team for this study are: Cristian Abelairas-Gomez, Katherine Allan, Jan Breckwoldt, Kathryn Eastwood, Ming-Ju Hsieh, Tracy Kidd, Ying-Chih Ko, Kasper G Lauridsen, Sabine Nabecker, Kevin Nation, Alexander Olaussen, Sebastian Schnaubelt, Taylor Sawyer, Chih-Wei Yang, and Joyce Yeung.

## Appendix A. Supplementary material

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.resplu.2025.100939>.

## Author details

on behalf of the Education Implementation Team Task Force of the International Liaison Committee on Resuscitation ILCOR<sup>1</sup> <sup>a</sup>*KidSIM-ASPIRE Simulation Research Program, Alberta Children's Hospital, University of Calgary, Calgary, Canada* <sup>b</sup>*Emergency Department, Calderdale & Huddersfield NHS Trust, Halifax, UK* <sup>c</sup>*School of Human and Health Sciences, University of Huddersfield, Huddersfield, UK* <sup>d</sup>*PICU, Children's Hospital of Philadelphia, Philadelphia, PA, USA* <sup>e</sup>*Faculty of Medicine, University of Bern, Bern,*

*Switzerland* <sup>f</sup>*Department of Surgical Science, University of Torino, Torino, Italy* <sup>g</sup>*Department of Precision Medicine in Medical, Surgical and Critical Care Area (Me.Pre.C.C.) University of Palermo, Palermo, Italy* <sup>h</sup>*Department of Anesthesia, Intensive Care and Emergency, Policlinico Paolo Giaccone Palermo Italy* <sup>i</sup>*Nursing, Midwifery and Allied Health Professional's Research Unit (NMAHP), Faculty of Health Sciences & Sport, University of Stirling, UK* <sup>j</sup>*Cochrane Singapore, Singapore Clinical Research Institute, Singapore* <sup>k</sup>*Department of Anesthesiology, Surgery and Medical Education, Vanderbilt University Medical Center, Nashville, TN, USA* <sup>l</sup>*Department of Emergency Medicine, Kyoto Prefectural University of Medicine, Kyoto, Japan* <sup>m</sup>*Department of Pediatrics and Emergency Medicine, Cumming School of Medicine, University of Calgary, Canada* <sup>n</sup>*KidSIM-ASPIRE Simulation Research Program, Alberta Children's Hospital, University of Calgary, Canada*

## REFERENCES

- Martin SS, Aday AW, Almarzooq ZI, et al. 2024 heart disease and stroke statistics: a report of US and global data from the American heart association. *Circulation* 2024;149:e347–913.
- Bray J, Howell S, Ball S, et al. The epidemiology of out-of-hospital cardiac arrest in Australia and New Zealand: a binational report from the Australasian Resuscitation Outcomes Consortium (Aus-ROC). *Resuscitation* 2022;172:74–83.
- Grasner JT, Herlitz J, Tjelmeland IBM, et al. European Resuscitation Council Guidelines 2021: Epidemiology of cardiac arrest in Europe. *Resuscitation* 2021;161:61–79.
- Kiguchi T, Okubo M, Nishiyama C, et al. Out-of-hospital cardiac arrest across the World: First report from the International Liaison Committee on Resuscitation (ILCOR). *Resuscitation* 2020;152:39–49.
- Soreide E, Morrison L, Hillman K, et al. The formula for survival in resuscitation. *Resuscitation* 2013;84:1487–93.
- Yang CW, Yen ZS, McGowan JE, et al. A systematic review of retention of adult advanced life support knowledge and skills in healthcare providers. *Resuscitation* 2012;83:1055–60.
- Cheng A, Magid DJ, Auerbach M, et al. Part 6: resuscitation education science: 2020 American heart association guidelines for cardiopulmonary resuscitation and emergency cardiovascular care. *Circulation* 2020;142:S551–79.
- Yeung J, Meeks R, Edelson D, Gao F, Soar J, Perkins GD. The use of CPR feedback/prompt devices during training and CPR performance: a systematic review. *Resuscitation* 2009;80:743–51.
- Panchal AR, Bartos JA, Cabanas JG, et al. Part 3: Adult basic and advanced life support: 2020 American heart association guidelines for cardiopulmonary resuscitation and emergency cardiovascular care. *Circulation* 2020;142:S366–468.
- Topjian AA, Raymond TT, Atkins D, et al. Part 4: pediatric basic and advanced life support: 2020 American heart association guidelines for cardiopulmonary resuscitation and emergency cardiovascular care. *Circulation* 2020;142:S469–523.
- Morley PT, Atkins DL, Finn JC, et al. Evidence evaluation process and management of potential conflicts of interest: 2020 international consensus on cardiopulmonary resuscitation and emergency cardiovascular care science with treatment recommendations. *Circulation* 2020;142:S28–40.
- Morley PT, Atkins DL, Finn JC, et al. Evidence evaluation process and management of potential conflicts of interest: 2020 international consensus on cardiopulmonary resuscitation and emergency cardiovascular care science with treatment recommendations. *Resuscitation* 2020;156:A23–34.



13. Page MJ, McKenzie JE, Bossuyt PM, et al. The PRISMA 2020 statement: an updated guideline for reporting systematic reviews. *PLoS Med* 2021;18:e1003583.
14. Sterne JAC, Savovic J, Page MJ, et al. RoB 2: a revised tool for assessing risk of bias in randomised trials. *BMJ* 2019;366:l4898.
15. Greif R, Bray JE, Djarv T, et al. 2024 international consensus on cardiopulmonary resuscitation and emergency cardiovascular care science with treatment recommendations: summary from the basic life support; advanced life support; pediatric life support; neonatal life support; education, implementation, and teams; and first aid task forces. *Circulation* 2024;150:e580–687.
16. Greif R, Bray JE, Djarv T, et al. 2024 international consensus on cardiopulmonary resuscitation and emergency cardiovascular care science with treatment recommendations: summary from the basic life support; advanced life support; pediatric life support; neonatal life support; education, implementation, and teams; and first aid task forces. *Resuscitation* 2024;205:110414.
17. Balduzzi S, Rucker G, Schwarzer G. How to perform a meta-analysis with R: a practical tutorial. *Evid Based Ment Health* 2019;22:153–60.
18. Allan KS, Wong N, Aves T, Dorian P. The benefits of a simplified method for CPR training of medical professionals: a randomized controlled study. *Resuscitation* 2013;84:1119–24.
19. Cortegiani A, Rusotto V, Montalto F, et al. Use of a real-time training software (Laerdal QCPR(R)) compared to instructor-based feedback for high-quality chest compressions acquisition in secondary school students: a randomized trial. *PLoS One* 2017;12:e0169591.
20. Ghaderi MS, Malekzadeh J, Mazloum S, Pourghaznein T. Comparison of real-time feedback and debriefing by video recording on basic life support skill in nursing students. *BMC Med Educ* 2023;23:62.
21. Gonzalez-Santano D, Fernandez-Garcia D, Silvestre-Medina E, et al. Evaluation of three methods for CPR training to lifeguards: a randomised trial using traditional procedures and new technologies. *Medicina (Kaunas)* 2020;56.
22. Jang TC, Ryoo HW, Moon S, et al. Long-term benefits of chest compression-only cardiopulmonary resuscitation training using real-time visual feedback manikins: a randomized simulation study. *Clin Exp Emerg Med* 2020;7:206–12.
23. Jiang J, Yan J, Yao D, et al. Comparison of the effects of using feedback devices for training or simulated cardiopulmonary arrest. *J Cardiothorac Surg* 2024;19:159.
24. Kardong-Edgren SE, Oermann MH, Odom-Maryon T, Ha Y. Comparison of two instructional modalities for nursing student CPR skill acquisition. *Resuscitation* 2010;81:1019–24.
25. Katipoglu B, Madziala MA, Evrin T, et al. How should we teach cardiopulmonary resuscitation?. *Randomized Multi-Center Study Cardiol J* 2021;28:439–45.
26. Kong SYJ, Song KJ, Shin SD, et al. Effect of real-time feedback during cardiopulmonary resuscitation training on quality of performances: A prospective cluster-randomized trial. *Hong Kong Journal of Emergency Medicine* 2020;27:187–96.
27. Labuschagne MJ, Arbee A, de Klerk C, et al. A comparison of the effectiveness of QCPR and conventional CPR training in final-year medical students at a South African university. *Afr J Emerg Med* 2022;12:106–11.
28. Lee PH, Lai HY, Hsieh TC, Wu WR. Using real-time device-based visual feedback in CPR recertification programs: A prospective randomised controlled study. *Nurse Educ Today* 2023;124:105755.
29. Lin Y, Cheng A, Grant VJ, Currie GR, Hecker KG. Improving CPR quality with distributed practice and real-time feedback in pediatric healthcare providers - A randomized controlled trial. *Resuscitation* 2018;130:6–12.
30. Meng XY, You J, Dai LL, Yin XD, Xu JA, Wang JF. Efficacy of a simplified feedback trainer for high-quality chest compression training: a randomized controlled simulation study. *Front Public Health* 2021;9:675487.
31. Min MK, Yeom SR, Yoo JH, et al. Comparison between an instructor-led course and training using a voice advisory manikin in initial cardiopulmonary resuscitation skill acquisition. *Clin Exp Emerg Med* 2016;3:158–64.
32. Pavo N, Goliasch G, Nierscher FJ, et al. Short structured feedback training is equivalent to a mechanical feedback device in two-rescuer BLS: a randomised simulation study. *Scand J Trauma Resusc Emerg Med* 2016;24:70.
33. Spooner BB, Fallaha JF, Kocierz L, Smith CM, Smith SC, Perkins GD. An evaluation of objective feedback in basic life support (BLS) training. *Resuscitation* 2007;73:417–24.
34. Suet G, Blanie A, de Montblanc J, Roulleau P, Benhamou D. External cardiac massage training of medical students: a randomized comparison of two feedback methods to standard training. *J Emerg Med* 2020;59:270–7.
35. Sutton RM, Niles D, Meaney PA, et al. “Booster” training: evaluation of instructor-led bedside cardiopulmonary resuscitation skill training and automated corrective feedback to improve cardiopulmonary resuscitation compliance of Pediatric Basic Life Support providers during simulated cardiac arrest. *Pediatr Crit Care Med* 2011;12:e116–21.
36. Wagner M, Bibl K, Hrdliczka E, et al. Effects of feedback on chest compression quality: a randomized simulation study. *Pediatrics* 2019;143.
37. Zhou XL, Wang J, Jin XQ, Zhao Y, Liu RL, Jiang C. Quality retention of chest compression after repetitive practices with or without feedback devices: a randomized manikin study. *Am J Emerg Med* 2020;38:73–8.
38. Jones A, Lin Y, Nettel-Aguirre A, Gilfoyle E, Cheng A. Visual assessment of CPR quality during pediatric cardiac arrest: does point of view matter?. *Resuscitation* 2015;90:50–5.
39. Cheng A, Overly F, Kessler D, et al. Perception of CPR quality: Influence of CPR feedback, Just-in-Time CPR training and provider role. *Resuscitation* 2015;87:44–50.
40. Ende J. Feedback in clinical medical education. *JAMA* 1983;250:777–81.
41. Rabanales-Sotos J, Guisado-Requena IM, Leiton-Espinoza ZE, et al. Development and validation of a novel ultra-compact and cost-effective device for basic hands-on CPR training: a randomized, sham-controlled, blinded trial. *Int J Environ Res Public Health* 2022;19.
42. Wang SA, Su CP, Fan HY, Hou WH, Chen YC. Effects of real-time feedback on cardiopulmonary resuscitation quality on outcomes in adult patients with cardiac arrest: A systematic review and meta-analysis. *Resuscitation* 2020;155:82–90.
43. Masterson S, Norii T, Yabuki M, et al. Real-time feedback for CPR quality - A scoping review. *Resusc plus* 2024;19:100730.
44. Sood N, Sangari A, Goyal A, et al. Do cardiopulmonary resuscitation real-time audiovisual feedback devices improve patient outcomes? A systematic review and meta-analysis. *World J Cardiol* 2023;15:531–41.
45. Merriam SB. Andragogy and self-directed learning: pillars of adult learning theory. *New Directions for Adult and Continuing Education* 2001;2001:3–14.
46. Young JQ, Van Merrienboer J, Durning S, Ten Cate O. Cognitive Load Theory: implications for medical education: AMEE Guide No. 86. *Med Teach* 2014;36:371–84.
47. Cook DA, West CP. Perspective: reconsidering the focus on “outcomes research” in medical education: a cautionary note. *Acad Med* 2013;88:162–7.
48. Vadeboncoeur T, Stolz U, Panchal A, et al. Chest compression depth and survival in out-of-hospital cardiac arrest. *Resuscitation* 2014;85:182–8.
49. Idris AH, Guffey D, Pepe PE, et al. Chest compression rates and survival following out-of-hospital cardiac arrest. *Crit Care Med* 2015;43:840–8.
50. Duval S, Pepe PE, Aufderheide TP, et al. Optimal combination of compression rate and depth during cardiopulmonary resuscitation for functionally favorable survival. *JAMA Cardiol* 2019;4:900–8.